

SUPPLEMENT ORIGINAL ISSUE

Precise Flight Oxygen System

Pilot's Operating Handbook
and
Airplane Flight Manual Supplement

Original Issue

Date: October 2, 2006

PFI Document Number: 102NMAN0001

Revision: B

Dated: May 30, 2008

**Insert the Following Pages Into The Supplement
Section Of
The Pilot's Operating Handbook**

This Page Intentionally Left Blank.

**Pilot's Operating Handbook and
FAA-Approved Airplane Flight Manual Supplement
For**

**Supplementary Type Certificate Number:
SA01708SE**

**Precise Flight, Inc.
Cirrus SR22 Fixed Oxygen System**

Aircraft Serial Number:	
Aircraft Registration Number:	

When supplemental oxygen is required by the applicable operating rules (FAR Part 23, FAR Part 91, or FAR Part 135), this Flight Manual Supplement ("Supplement") is applicable and must be inserted in Section 9 of the Pilot's Operating Handbook ("Handbook"). Information in this Supplement adds to, supersedes, or deletes information in the basic handbook.

FAA-APPROVED

Donald B. Wilson

DATE

May 30, 2008

for Jeff Duvon, Manager
Seattle Aircraft Certification Office
Federal Aviation Administration

Fixed Oxygen System

Table of Revisions

Use the Table of Revisions to determine the current status of this Supplement. Pages affected by the current revision are indicated by an asterisk (*) preceding the page number.

This Supplement is an addition to the primary FAA-Approved Flight Manual Supplement / Pilots Operating Handbook (AFM/POH) and contains the same sections as found in the Primary document. This table summarizes the applicable revisions by page number.

Revision Level/ Date	Page	Revision Level/ Date	Page	Revision Level/ Date	Page	Revision Level/ Date	Page
B / 5/30/08	1	B / 5/30/08	11	B / 5/30/08	21	B / 5/30/08	31
B / 5/30/08	2	B / 5/30/08	12	B / 5/30/08	22	B / 5/30/08	32
B / 5/30/08	3	B / 5/30/08	13	B / 5/30/08	23	B / 5/30/08	33
B / 5/30/08	4	B / 5/30/08	14	B / 5/30/08	24	B / 5/30/08	34
B / 5/30/08	5	B / 5/30/08	15	B / 5/30/08	25	B / 5/30/08	35
B / 5/30/08	6	B / 5/30/08	16	B / 5/30/08	26	B / 5/30/08	36
B / 5/30/08	7	B / 5/30/08	17	B / 5/30/08	27	B / 5/30/08	37
B / 5/30/08	8	B / 5/30/08	18	B / 5/30/08	28	B / 5/30/08	38
B / 5/30/08	9	B / 5/30/08	19	B / 5/30/08	29		
B / 5/30/08	10	B / 5/30/08	20	B / 5/30/08	30		

Service Bulletin Configuration List

The following is a list of service bulletins applicable to the operation of the airplane, and have been incorporated into this Supplement. This list contains only those service bulletins that are currently active.

Number	Title	Airplane Serial Effectivity	Revision Incorporated	Incorporated in Airplane

Table of Contents

Table of Revisions	2
Service Bulletin Configuration List.....	2
Table of Contents.....	3
Section 1 – General System Overview	4
1.1 – OPTIONAL – Cirrus Perspective by Garmin.....	7
1.2 – Constant Flowmeters	12
1.3 – PreciseFlow® Oxygen Conservers (PFOC)	14
1.4 – OPTIONAL – Pulse Oximeter (FlightStat)	22
Section 2 – Limitations.....	24
Section 3 – Emergency Procedures	26
3.1 – General	26
3.2 – Smoke and Fume Elimination	26
Section 4 – Normal Procedures	27
4.1 – General	27
4.2 – Preflight	27
4.3 – Before Starting Engine (If oxygen is required or preferred).....	28
4.4 – In Route (if oxygen is required or preferred).....	28
4.5 – Shutdown (if oxygen is required or preferred)	29
Section 5 – Performance	30
5.1 – Oxygen Bottle Capacity vs Pressure	30
5.2 – A4 Constant Flow Meter with Standard Cannula or Constant Flow Mask.....	31
5.3 – A5 Constant Flow Meter with Standard Cannula or Constant Flow Mask.....	32
5.4 – PreciseFlow Oxygen Conserver (PFOC) Normal Operation.....	33
Section 6 – Weight & Balance	34
Section 7 – System Description.....	34
Section 8 – Handling, Service, & Maintenance	35
8.1 – Refilling the Oxygen Bottle.....	35
8.2 – Oxygen Component Cleaning.....	35
8.3 – Oxygen Bottle Removal	36
8.4 – Replacement Components	37

Fixed Oxygen System

Section 1 – General System Overview

This Supplement provides information that should be observed when operating the Precise Flight, Inc. Fixed Oxygen System. The System is designed to provide supplemental oxygen for the pilot and passengers. The System consists of a 77 cu ft bottle and a pressure regulator assembly located in the aft fuselage, a four (4)-place distribution manifold located in the headliner, a control panel located in the center console next to the flap switch, a filler port with a manual pressure gage located in the aft wall of the baggage compartment, related oxygen lines and System electrical lines, and up to four (4) flow devices consisting of either constant flow meters, or demand regulators, with either a cannula or face mask for each user.

The FAA Approved flow devices consist only of Precise Flight A4 or A5 constant flowmeters, or the Precise Flight demand flow conserver. The A4 and A5 flowmeters are constant flowmeter options that are calibrated and adjustable for altitude to supply oxygen to either oxygen conserving cannulas, standard cannula, up to 18,000ft, or masks for altitudes up to the maximum operating altitude of the Cirrus SR22 or 25,000ft whichever is less. The PreciseFlow[®] demand flow conservers are calibrated and adjusted by the user for altitude to supply oxygen to either dual lumen cannulas up to 18,000ft, or dual sensing masks for use to altitudes up to the maximum operating altitude for the Cirrus SR22 or 25,000ft whichever is less.

■ Note ■

Facemasks covering the nose and mouth are required above 18,000ft per 14 CFR Part §23.1447.

The cockpit control electrically actuates the regulator allowing oxygen flow into the aircraft cabin. The cockpit control will annunciate O2 REQ'D if the System is not selected ON and the aircraft is above approx. 12,000ft PA to alert the requirement of oxygen in the cabin. Once the oxygen is selected ON, the quantity display illuminates indicating the presence of oxygen in the cabin.

System faults are indicated by the FAULT annunciator. Steady fault indication signifies a problem with the aircraft wiring and will disable the

System. When a steady fault indication is present, the System is disabled and will not reset until power is cycled to the controller. This can be done by cycling the OXYGEN / CABIN LTS circuit breaker, or by cycling aircraft power. Flashing LED FAULT indication specifies an oxygen pressure fault to the distribution manifold. The oxygen quantity display will flash red if the bottle pressure falls below 400 psig.

■ **Note** ■

When the System is first engaged, the FAULT light may briefly flash until proper pressure is sensed at the overhead distribution manifold. This is normal, as pressure may bleed off when not in use.

■ **Note** ■

In the event of an electrical failure on Main Bus 2, oxygen will remain on in the cabin. Aircraft electrical power is required ONLY to turn the System ON and OFF. The System is designed to remain ON during an electrical failure, but oxygen quantity indication will be lost. Disconnecting the lines from the manifold will prevent the free flow of oxygen in the cabin.

Prior to flight, the pilot should turn System ON to ensure sufficient oxygen quantity (pressure) exists for the flight and for passenger requirements using the duration charts included in this Supplement. The System is selected ON at the oxygen control at pilot discretion to meet personal physiological or FAA flight rule requirements. The System requires the user(s) don an Oxymizer cannula, a standard cannula, or an oxygen mask for the constant flowmeters. All users will subsequently set the flowmeter ball to the pressure altitude, or the altitude knob on the PreciseFlow[®], indicated on the primary flight display, or above that altitude to meet the pilot or passenger physiological requirements if additional oxygen is needed.

The flow devices provide the means to distribute the appropriate amount of oxygen for the pressure altitude of flight and indicate the presence of flowing oxygen to the pilot and users. All flow devices must be checked periodically (recommended intervals of less than 10 min.) to ensure flow and correct settings, as well as the oxygen control panel quantity indication.

All delivery systems must be properly set to the corresponding altitude with each change in pressure altitude.

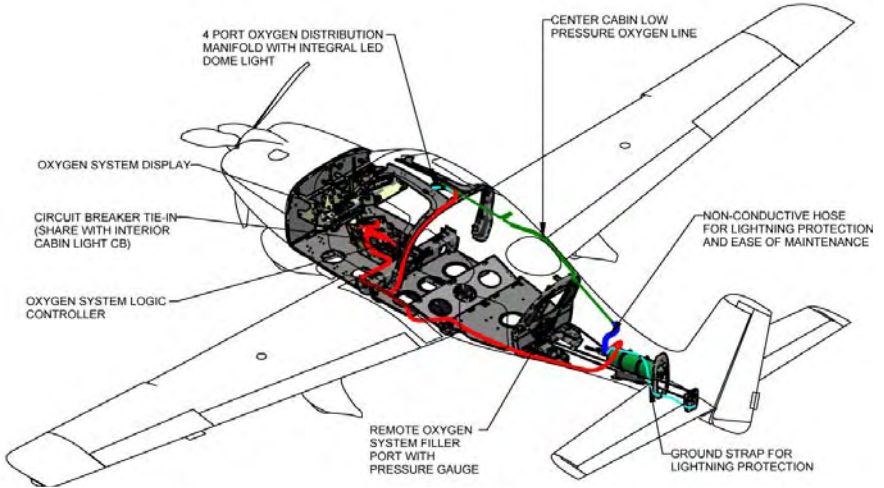


Figure 1 – Oxygen System Installation



Figure 2 – Oxygen Control Panel

1.1 – OPTIONAL – Cirrus Perspective by Garmin

■ Note ■

This section is for information only.

The primary oxygen information display is the Oxygen Display Panel in the center console to the left of the flap switch.

Please refer to the Garmin P/N: 190-00820-00 “The Cirrus Perspective by Garmin Integrated Avionics System Pilot’s Guide for the SR22” Original Release or Later Approved Document for full Garmin interface information.

An optional output is provided from the Precise Flight Oxygen System Display/Logic Controller located in the center console that provides pressure (quantity), indication, and warning signals to the Garmin GEA 71 airframe interface on the Garmin G1000 equipped aircraft for secondary information only.



Figure 3 - Optional Garmin GEA 71

The primary oxygen system display is provided by the oxygen display located in the Integrated Flap Panel to the left of the Flap Switch. The display looks similar to that shown in Figure 2. In the Cirrus Perspective, the display text is back-lit and dim control is provided with the aircraft dim control.

With this option installed, the MFD engine page displays the Oxygen Bottle Pressure (high pressure) that directly indicates oxygen Quantity as shown in Figure 4, and detailed in Figure 5.



Figure 4 - Garmin G1000 MFD Engine Page



Figure 5 - G1000 MFD Oxygen Pressure Indicator Detail

1.1.1 – EIS Display in Reversionary Mode

Secondary pressure indication is provided on the System Display side display when in reversionary mode as shown in Figure 6.





Figure 6 - Reversionary Mode System Display




1.1.2 – Oxygen System Aircraft Alerts

■ WARNING ■

The G1000 Aircraft Alerts are considered Secondary Annunciation and the primary warning and advisory annunciation is provided on the Oxygen System Display.

The Garmin display will display a steady caution  when the bottle pressure is between 400psig-800psig, and the Garmin MFD engine page oxygen quantity gauge has a caution (amber) marking between 400psig-800psig. This is different than the primary display located next to the flap switch which will show green indication from 400psig-800psig.

The Garmin display will display a steady warning  when the bottle pressure is less than 400psig. This is different than the primary display located next to the flap switch which will show a flashing red EMPTY light at below 400psig.

The Garmin display will only display the Oxygen warnings  , or Caution  when the system is ON, or the aircraft is above 10,000ft, and the conditions exist for the warning. This is different than the primary display which will not display pressure, or pressure warnings, unless the system is ON.

Both systems will provide the Oxygen Required warning if the system is OFF, or there is insufficient outlet pressure with the system ON, above 12,000ft PA.

The Garmin G1000 provides secondary annunciation on the PFD in the Alerts Window with Audio Alerts. These alerts are either Warning or Cautions as shown in Figure 7, Table 1, and Table 2.



Figure 7 - G1000 Warning and Caution Alerts

Oxygen System Warnings include system Faults indicating an electrical or outlet pressure fault. Low Oxygen Quantity is also considered a Warning on the G1000 as these indicators show a oxygen system fault or condition that will prevent proper oxygenation. The Oxygen Quantity Warning is displayed when the quantity drops below 400psi.

Table 1 - Oxygen System Warning Alerts

Annunciation Window Text	Alerts Window Text	Audio Alert
OXYGEN FAULT⁺	Oxygen System Fault	Repeating Double Chime
OXYGEN QTY⁺	Oxygen Quantity is Low (<400psig)	Repeating Double Chime

Oxygen System Cautions include the advisory information such as Oxygen Required as indicated by the Oxygen System when the system is not providing pressure (Low pressure or system OFF) at the distribution manifold and the PS is 12,000+-500ft. Oxygen Quantity caution is also displayed with the quantity drops below 800psi.

Table 2 - Oxygen System Caution Alerts

Annunciation Window Text	Alerts Window Text	Audio Alert
OXYGEN QTY⁺	Oxygen Quantity is Low (400psig-800psig)	Double Chime
OXYGEN RQD⁺	Oxygen is Required	Double Chime

1.2 – Constant Flowmeters

The constant flowmeters are calibrated and adjustable for altitude to supply oxygen to either oxygen conserving, or standard, cannulas up to a maximum altitude of 18,000ft MSL, or masks for altitudes up to a maximum of altitude of 25,000ft MSL , or the maximum operating altitude of the aircraft whichever is lower.. The System requires the pilot and passengers to don either an Oxyimizer cannula, standard cannula, or an oxygen mask first, then the pilot and passengers will open the oxygen valve, noting oxygen quantity, and subsequently set the flowmeter ball to the pressure altitude chosen for flight, or at a setting above the altitude chosen to meet the physiological requirements of the pilot.



Figure 8 – A4 Constant Flow
Oxygen Flowmeter



Figure 9 – A5 Constant Flow
Oxygen Flowmeter

The flowmeters provide the means to distribute the appropriate amount of oxygen for the pressure altitude of flight and indicate the presence of oxygen flowing to the pilot and/or passengers. The flowmeter should be checked periodically (recommended intervals of less than 10 min) as well as the oxygen quantity gauge. The flowmeter should be readjusted with each change in pressure altitude or physiological requirement.

This Supplement is applicable when supplemental oxygen is required by the applicable operating rules, and provides mounting instructions.



Figure 10 – Oxygen Flowmeter

■ Caution ■

Use of cannulas is recommended only for persons with a demonstrated ability to be properly oxygenated using these types of delivery devices. Precise Flight, Inc. encourages the use of a pulse oximeter while using a supplemental oxygen system, as a person's physiological differences may alter oxygen saturation, and these effects may change day-to-day depending on health or respiratory challenges such as allergies, etc.

■ Note ■

When using a face mask, ensure a tight seal around the face.
Users with facial hair should not use a face mask.

1.3 – PreciseFlow® Oxygen Conservers (PFOC)

The PreciseFlow® Oxygen Conserver is a Demand Regulator calibrated and adjustable for altitude to supply oxygen to Standard Dual Lumen Cannulas up to a maximum altitude of 18,000ft MSL, or Dual Supply PFOC Masks up to a maximum operating altitude of 25,000ft MSL, or the maximum operating altitude of the aircraft whichever is lower. The system requires the pilot to don either a Dual Lumen Cannula or a PFOC Mask first, then the pilot will open the Oxygen Valve, noting oxygen quantity, and subsequently set the Altitude Dial to the pressure altitude chosen for flight, or at a setting above the altitude chosen to meet the pilot physiological requirements. Additionally the PreciseFlow® Oxygen Conserver can be set to constant flow for additional oxygen when required.

■ **Note** ■

Facemasks covering the nose and mouth are required above 18,000ft MSL per 14 CFR Part §23.1447.

■ **Note** ■

PreciseFlow® with Inline Regulator must be used with the Cirrus SR22 built in system.



**Figure 11 - PreciseFlow® Oxygen Conserver Breathing Station Kit
(with Dual Lumen Cannula and Standard Dual Supply Mask Shown)**

There are three major reasons for using the PreciseFlow® Oxygen Conserver on a general aviation aircraft. One is the conservation of

oxygen, allowing smaller portable or fixed oxygen bottles to be used or to increase the duration of usable oxygen for a given volume. The second is that the manner of delivery for a demand conserver is physiologically better. Third being that interrupted flow is better for the users nasal passages.

Conservation - Utilizing demand flow and interrupting the flow of oxygen can provide a potential savings of 3 fold over continuous flow systems. The three fold savings is derived from a standard breathing cycle with 1/3 of the cycle being inhalation and exhalation taking the remaining 2/3. The PreciseFlow conserver defaults to constant flow with rapid breathing (breathing over 22 breaths per minute) as hysteresis in the mechanical system defaults the unit to constant flow.

Delivery – The ability to deliver a bolus of oxygen improves oxygen saturation by allowing the first air of the inhalation cycle to be more fully enriched with oxygen. It is this gas that participates in gas exchange in the lungs with the remainder of the breath providing the pressure to allow the gas to exchange across the lung surface into the blood. This bolus of oxygen can be felt and encourages the user to breath through the nose.

Comfort – The ability to interrupt flow keeps the dry oxygen gas from flowing over the nasal passages continually. The lack of dry gas flow allows the nasal passages to remain moist. The comfort level encourages oxygen usage for people with sensitivity to nasal discomfort.

The PreciseFlow[®] Oxygen Conserver provides the means to efficiently distribute the appropriate amount of oxygen for the pressure altitude of flight, and indicate the presence of flowing oxygen to the pilot or passengers. The PreciseFlow[®] Oxygen Conserver Flow Indicator and oxygen quantity gauge should be checked periodically at an interval of no more than every 10 min. The PreciseFlow[®] Oxygen Conserver should be set for each change in pressure altitude or for personal physiological requirements. This supplement is applicable when supplemental oxygen is required by the applicable operating rules, and provides mounting instructions.

The different mode combinations for the PreciseFlow[®] Oxygen Conserver unit are shown in Figure 12 where the first picture shows a typical operation setting for flight between 16,000ft and 22,000ft. The unit is set to conserve using the mode select dial, and the altitude is set

to '16K'. Instructions provided to the user state that the PreciseFlow[®] Oxygen Converter should be adjusted to the next higher altitude from where flight is being conducted. Above 18,000 ft where a mask is required, **constant** flow is to be selected with a dual supply mask as indicated with a box around the altitudes on the altitude selection knob, and the 'constant' on the mode select knob. If physiological requirements differ for the user, the 'constant' mode, or a higher altitude setting may be selected at any altitude. The **THP** setting is calibrated to flow 4LPM of Oxygen. This far exceeds the minimum flow requirement of 2.3LPM at 25,000ft should additional oxygen be required by the user.

The conserve mode process is accomplished by an internal flow control disk that controls the flow of oxygen and a valve system controlled on the inhalation and exhalation cycles of the user within the unit. This breath cycle is sensed through the use of a dual lumen cannula, or the dual port mask. A calibrated orifice controls the flow rate is set by the altitude knob at the end of the unit.

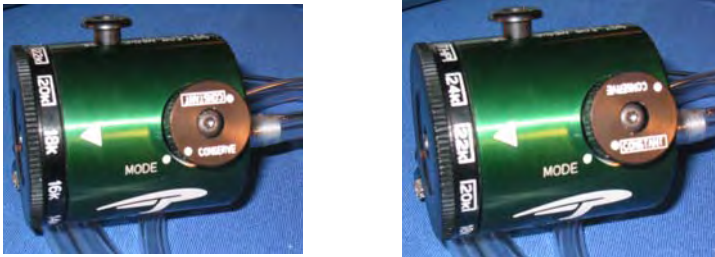


Figure 12 – PreciseFlow[®] Oxygen Converter – Mode Combinations

■ **Caution** ■

Use of cannulas recommended only for person who have demonstrated the ability to be properly oxygenated with these delivery devices. Precise Flight Inc. encourages the use of a pulse oximeter while using supplemental oxygen system as peoples physiological differences can alter oxygen saturations from person to person.



Figure 13 – PreciseFlow® Oxygen Conserving

1.3.1 – Dual Lumen Cannula Use

The Dual Lumen Cannula (See Figure 14) is for use with the PreciseFlow® Oxygen Converter only, and should not be used with other breathing equipment. This cannula is unique in that it provides both oxygen delivery and sensing to the PreciseFlow® Oxygen Converter. The sensing port is required to provide a pressure drop to the PreciseFlow® during inhalation, signaling the converter to provide oxygen through the deliver line.



Figure 14 - Dual Lumen Cannula

First attach the Dual Lumen Cannula to the PreciseFlow® Oxygen Converter, one tube connector to the **Delivery** side, and the other to the **Sensing** side as shown in Figure 15.



Figure 15 - Attachment of the Dual Lumen Cannula to the PreciseFlow® Oxygen Converter

1. Please make sure you are wearing the cannula with the tab pointing down (found at the base of the nasal prongs - see Figure 16).

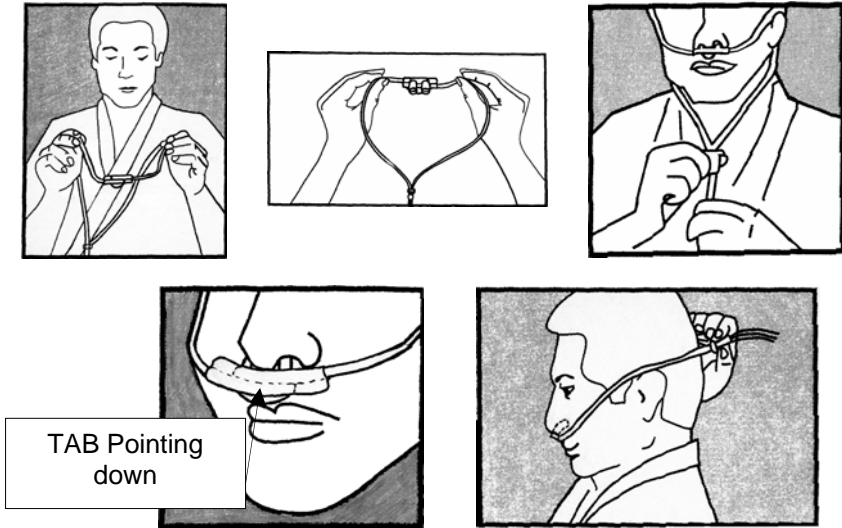


Figure 16 - PreciseFlow Conserver Cannula Usage

2. Flow can be restricted if the small diameter tubes that lead to the nasal prongs on the cannula get pinched under a headset. The best solution is to put the cannula on over your headset so the tubes rest on the outside of the earpieces.
3. Adjust the PreciseFlow Oxygen Conserver to the desired altitude and breathe through the nose.

■ **Note** ■


Proper Oxygenation above 16,000 feet using the PreciseFlow Conserver and Dual Lumen cannula requires deliberate and consistent deep breathing through the nose.

■ **Note** ■

Cannulas are limited to a maximum altitude of 18,000ft MSL per 14 CFR Part §23.1447.

1.3.2 – Dual Supply Demand Mask Use

There are two dual supply mask options for use with the PreciseFlow Oxygen Conservser.

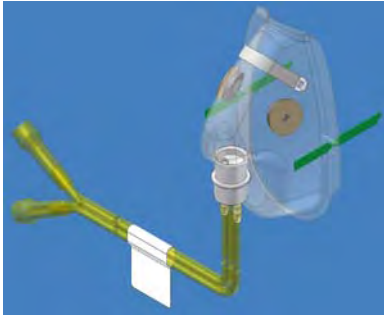

**Figure 17 – Dual Supply
Standard Mask**



**Figure 18 – Dual Supply Mask
with Microphone**

To use a facemask, the PreciseFlow Oxygen Conservser must be set in the “**Constant**” flow mode. First attach the Dual Supply Mask to the PreciseFlow Oxygen Conservser, one tube connector to the **Delivery** side, and the other to the **Sensing** side as shown in Figure 19.



**Figure 19 - Attachment of the Dual Lumen Cannula to the
PreciseFlow Oxygen Conservser**

Wear the Face Mask per the instructions provided with the mask, and check the flow indicator to ensure that oxygen is flowing through the system.

■ **Note** ■

Do not use the PreciseFlow Oxygen Conserver with a bag reservoir Face Mask. Only Precise Flight Face Masks with a delivery and sensing line are approved for use with the PreciseFlow Conserver.

■ **Note** ■

When using a Face Mask, ensure a tight seal around the face. Users with Facial hair should not use a Face Mask.

■ **Caution** ■

Use of cannulas is recommended only for persons with a demonstrated ability to be properly oxygenated using these types of delivery devices. Precise Flight, Inc. encourages the use of a pulse oximeter (See Section 1.3) while using a supplemental oxygen system, as a person's physiological differences may alter oxygen saturation, and these effects may change day-to-day depending on health or respiratory challenges such as allergies, etc.

1.4 – OPTIONAL – Pulse Oximeter (FlightStat)

■ Caution ■

Pulse Oximetry will read Carbon Monoxide as Oxygen and show false level of oxygen saturation.

■ Caution ■

This is a tool, and not a replacement for diligence of the user to notice the physiological signs of the onset of hypoxia caused by lack of oxygen, carbon monoxide poisoning, or other factors.

The Nonin Medical “FlightStat” Pulse Oximeter (Figure 20 / Figure 21) emits red and infrared light through the finger and detects the fluctuating signals caused by the pulsating blood flow. Pulse rate is determined from the signals received by a light detector. The ratio of the fluctuation between red and infrared light signals is used to calculate the relative blood oxygen saturation (%SpO₂) of hemoglobin. A pulse oximeter indicates what percent of hemoglobin molecules are carrying oxygen; blood oxygen saturation or %SpO₂. A %SpO₂ reading of 97 indicates that a relative 97% of your hemoglobin molecules are carrying oxygen.

At higher altitudes, %SpO₂ decreases due to less oxygen available because of the decrease in air pressure. Physical exertion at high altitude may be difficult because of the reduced oxygen level.



Figure 20 – FlightStat Pulse Oximeter

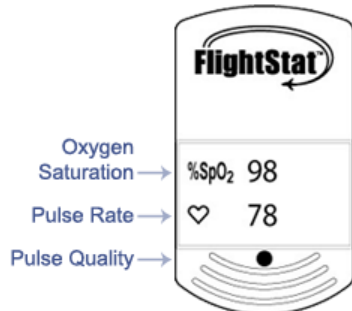


Figure 21 - FlightStat Key Features

Two AAA-size batteries power the FlightStat for approximately 1,600 spot checks; it may be stored for approximately nine months. When the batteries are low, the numeric displays flashes once per second. To conserve battery life, the FlightStat will automatically shut off approximately ten seconds after the finger is removed.

This unit's advanced digital circuitry requires no calibration or periodic maintenance other than periodic battery replacement.

1.3.1 - How to Use and Read the FlightStat

It is important to understand what each symbol and display means (See Figure 20):

Blood Oxygen Saturation: Displays the relative %SpO₂ of blood.

Pulse Rate: Displays the number of pulses per minute.

Pulse Quality: Blinks green, yellow, or red to indicate changes in pulse quality.

Inserting a finger into the FlightStat will automatically activate the device. Once the unit has been activated and has had time to determine the relative %SpO₂ and pulse rate, the information is displayed. Precise Flight recommends periodic checks of the crew and passengers during flight at altitude, and adjusting oxygen use accordingly by increasing the altitude setting if a person feels any effects of hypoxia, or if the oxygen saturation is low.

■ Note ■

The FlightStat must be used on a bare finger without gloves, bandages, etc. as it requires a clear light path through the finger to properly function.

Section 2 – Limitations

The installation of this equipment does not affect or change the limitations of the airplane, which are detailed in Section 2 of the primary portion of the AFM/POH. However, the following limitations apply to operation of the Fixed Oxygen System.

1. Oxyimizer Cannula and A4 or A5 Flowmeter to be used up to 18,000ft MSL ONLY.
2. Standard Cannula and A4 or A5 Flowmeter to be used up to 18,000ft MSL ONLY.
3. Dual Lumen Cannula and a PreciseFlow[®] to be used up to 18,000ft MSL ONLY.
4. An appropriate mask with the A4 or A5 Flowmeter must be used by persons experiencing nasal congestion, and above 18,000 ft MSL and up to 25,000ft MSL.
5. Oxygen mask and A4 or A5 Flowmeter or PreciseFlow[®] to be used up to 25,000ft MSL ONLY.
6. The PreciseFlow[®] to be used with a PFOC Mask and in Constant Mode ONLY above 18,000ft up to and including 25,000ft
7. Smoking is not permitted in any aircraft with oxygen in use.
8. Placards – On the individual oxygen masks and cannulas.

■ **WARNING** ■

Do not use oxygen while utilizing lipstick, Chapstick, petroleum jelly or any other product containing oil or grease.

■ **WARNING** ■

Smoking is not permitted while using the Oxygen System.

■ **Note** ■

If the aircraft is being operated under IFR and the pilot has nasal congestion, a mask containing a microphone should be used.

The following oxygen systems dispensing units are approved for use:

Table 3 – FAA-Approved Cirrus Fixed Oxygen System Components

Supplier	Capacity	Delivery Options	Dispensing Unit Options
Precise Flight, Inc. Bend, Oregon, United States of America	77 cuft	A4 A5	Oxymizer Cannula Standard Cannula Standard Constant Flow Mask Microphone Constant Flow Mask
		PFOC with Inline Regulator	Dual Lumen Cannula PFOC Standard Mask PFOC Microphone Mask
* STC Installation Kits noted, Dispensing Units listed may be replaced individually by the Precise Flight, Inc. Products listed. See Table 5 for specific PFI part number options.			

■ **Note** ■

The FAA, under 14 CFR Part 23 Regulations, require the complete Oxygen System (including the breathing stations, flowmeters, cannulas, and masks) be certified as a complete System. The use of other breathing equipment in conjunction with the built-in portion of the System has not been tested, nor is it FAA-Approved.

■ **Note** ■

PreciseFlow[®] with Inline Regulator must be used with the Cirrus SR22 built in system.

Section 3 – Emergency Procedures

3.1 – General

If the Precise Flight Oxygen System ceases to provide adequate oxygen for the altitude indicated on the flowmeter, safely descend immediately below 12,500ft PA. Close the oxygen supply valve.

If the System indicates a pressure or electrical malfunction on the FAULT annunciator or the System is not performing properly, do not attempt to identify or analyze the problem. Safely descend immediately below 12,500ft PA. Turn Oxygen System OFF.

The installation of this equipment does not affect or change the emergency procedures of the airplane, which are detailed in Section 3 of the primary portion of the Pilot's Operating Handbook.

1. Oxygen OFF or as required for smoke in the cabin.
2. Oxygen OFF for a cabin fire.

■ Caution ■

It is the pilot's responsibility to safely descend to a lower altitude. The pilot may have to reroute flight path to avoid terrain or other hazards.

3.2 – Smoke and Fume Elimination

In addition to the procedures outlined in the basic handbook, pilot and passengers should don masks and use oxygen at the maximum flow rate until smoke and fumes have cleared.

■ Note ■

The pilot must use their discretion in oxygen use as not to cause a hazard in the event of an in-cabin fire.

Section 4 – Normal Procedures

4.1 – General

The normal procedures for takeoff, climb, cruise, descent, and landing, which are detailed in Section 4 of the Pilot's Operating Handbook should be used. The following additional items must be incorporated into the normal checklists as applicable when the Oxygen System is in-use. The installation of this equipment does not affect or change the normal procedures or performance of the airplane, which is detailed in Section 4 of the primary portion of AFM/POH, except as noted above.

■ **Note** ■

Refer to Section 5 - Performance for duration at various altitudes and passengers using oxygen.

4.2 – Preflight

1. Oxygen Control..... Switch to ON
 - a. Check Quantity..... Enough for Planned Flight with Reserve
 - b. Outlet Pressure Ensure Pressure at Distribution Manifold
2. Oxygen Masks or Cannulas Check for Rips, Tears, or Blockage
3. Oxygen Masks or Cannulas Connected to Regulator
4. Flowmeter (If Applicable)..... Internal Ball Moves when Held Vertical
5. PreciseFlow[®] (If Applicable)..... Flow indicator indicating flow during breath cycle.
6. Oxygen Control..... OFF – If Oxygen is not required or preferred.

■ **Note** ■

The flowmeter must be held vertically when adjusting flow rate or reading.

■ **Note** ■

Reading is taken at the midpoint of the ball.

4.3 – Before Starting Engine (If oxygen is required or preferred)

1. PassengersBrief on Oxygen System operation.

■ **Note** ■

Briefing to include oxygen mask/cannula donning, flowmeter and/or PreciseFlow[®] adjustment, and connection to oxygen bottle regulator.

2. Oxygen Masks & Cannulas Don
3. Flowmeter (If Applicable)..... Set to the intended cruise altitude.
4. PreciseFlow[®] (If Applicable) Set to Intended Cruise Altitude

4.4 – In Route (if oxygen is required or preferred)

1. Flowmeter (If Applicable) Periodically check the flowmeter.

■ **Note** ■

Check the flowmeter or flow indicator at intervals of less than every 10 min intervals to ensure proper settings.

■ **Note** ■

The flowmeter must be held vertically when adjusting flow rate or reading.

■ **Note** ■

Reading is taken at the midpoint of the ball.

2. Flowmeter (If Applicable) Adjust as necessary.
3. PreciseFlow[®](If Applicable)Periodically Check the Flow Indicator
4. PreciseFlow[®](If Applicable) Adjust as Necessary
5. Flexible Oxygen Lines Ensure free flow of oxygen.
6. Pilot & PassengersLimit conversation.
7. Pilot & PassengersBreath through the nose if using a cannula or face mask.

■ **Note** ■

If an electrical fault has been detected during flight, the OXYGEN/CABIN LTS circuit breaker must be reset to operate the oxygen system.

4.5 – Shutdown (if oxygen is required or preferred)

1. Oxygen Control OFFClose
2. Flowmeter (If Applicable)..... Leave open until pressure is relieved
3. PreciseFlow®(If Applicable) Turn to Constant Mode
to Relieve Pressure
4. Lines, Flowmeters, PreciseFlow® and Masks Stow safely
until next flight.

■ **Note** ■

The flexible oxygen line in the aft fuselage compartment that is utilized to provide lightning protection for the Oxygen System is not gas tight in that the small oxygen molecules will slowly leak through this line. Ensure the Oxygen System is turned OFF prior to aircraft shutdown to preserve oxygen quantity.

Section 5 – Performance

Oxygen duration charts in this section are provided below for flight planning purposes. The installation of this equipment does not affect or change the performance characteristics of the airplane, which are detailed in Section 5 of the primary portion of the AFM/POH.

5.1 – Oxygen Bottle Capacity vs Pressure

Following Boyle's law, the bottle pressure vs capacity is linear thus the actual quantity left (bottle Pressure) can be noted and the duration charts in this section adjusted.

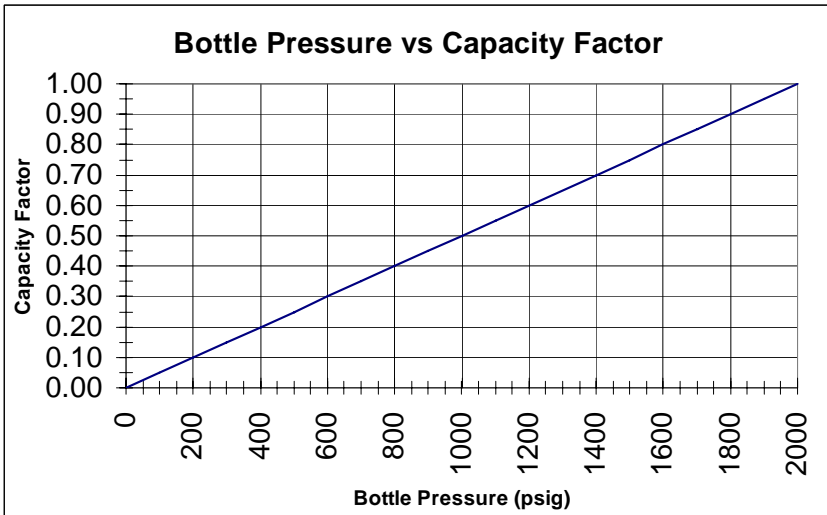


Figure 22 - Bottle Pressure/Capacity Factor Graph

EXAMPLE:

The pilot and 1 passenger are planning a flight at 16,000ft, using 2 PFOC Demand Conservers in the Conserver Mode with a Bottle Pressure of 1500psig. What is the available duration at this setting?

From Figure 22, for 1500psig the Capacity Factor is 0.75. From Figure 25 the duration for two active users is 17hrs. The duration available is calculated by multiplying the duration by the Capacity Factor.

Thus the actual available duration is $17\text{hrs} * 0.75 = 12.75\text{hrs}$ for this flight.

5.2 – A4 Constant Flow Meter with Standard Cannula or Constant Flow Mask

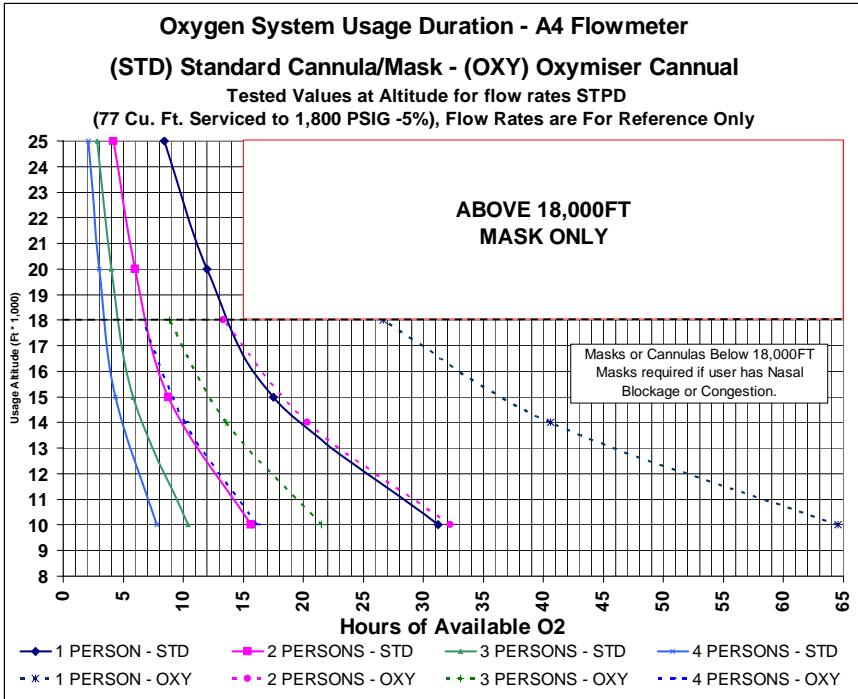


Figure 23 - A4 Flowmeter (Oxymizer and STD Scales)

Duration Chart Notes:

- Duration chart values are based on a 77 cu ft bottle capacity.
- Residual oxygen below 200 PSI has been factored out of the total oxygen quantity.
- Bottle capacity has been reduced five percent for safety.
- The installation of this equipment does not affect or change the performance characteristics of the airplane, which are detailed in Section 5 of the primary portion of the Pilot's Operating Handbook. No change from the basic handbook.

5.3 – A5 Constant Flow Meter with Standard Cannula or Constant Flow Mask

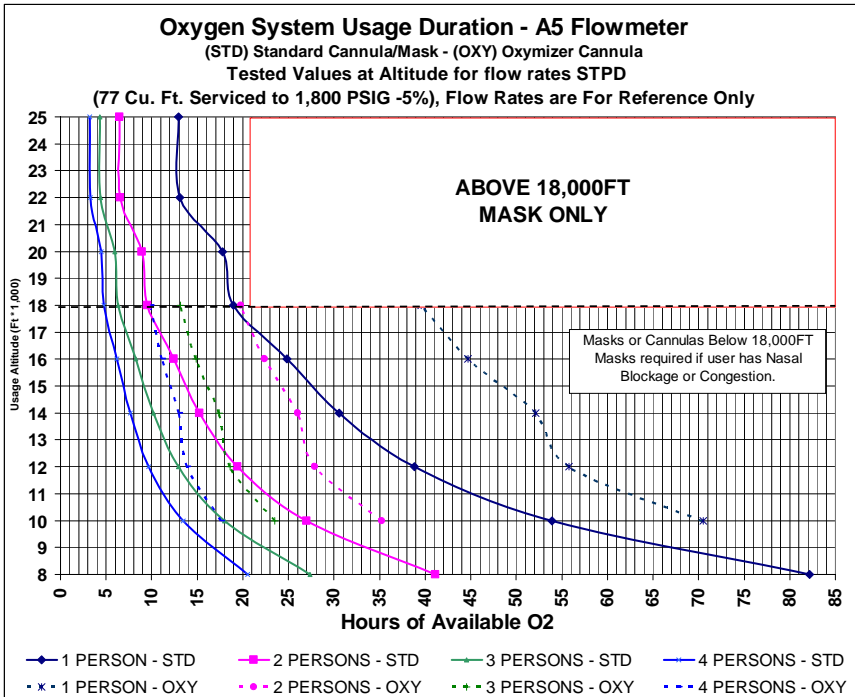


Figure 24 - A5 Flowmeter (Oxymizer and Standard Scales)

Duration Chart Notes:

- Duration chart values are based on a 77 cu ft bottle capacity.
- Residual oxygen below 200 PSI has been factored out of the total oxygen quantity.
- Bottle capacity has been reduced five percent for safety.
- The installation of this equipment does not affect or change the performance characteristics of the airplane, which are detailed in Section 5 of the primary portion of the Pilot's Operating Handbook. No change from the basic handbook.

5.4 – PreciseFlow Oxygen Conservser (PFOC) Normal Operation

■ Note ■

Pilot should calculate flow consumption based on Active use for flight crew. Actual flow consumption rates will vary from person to person when in conserve mode.

■ Caution ■

Mask and Constant Flow Mode required above 18,000ft.

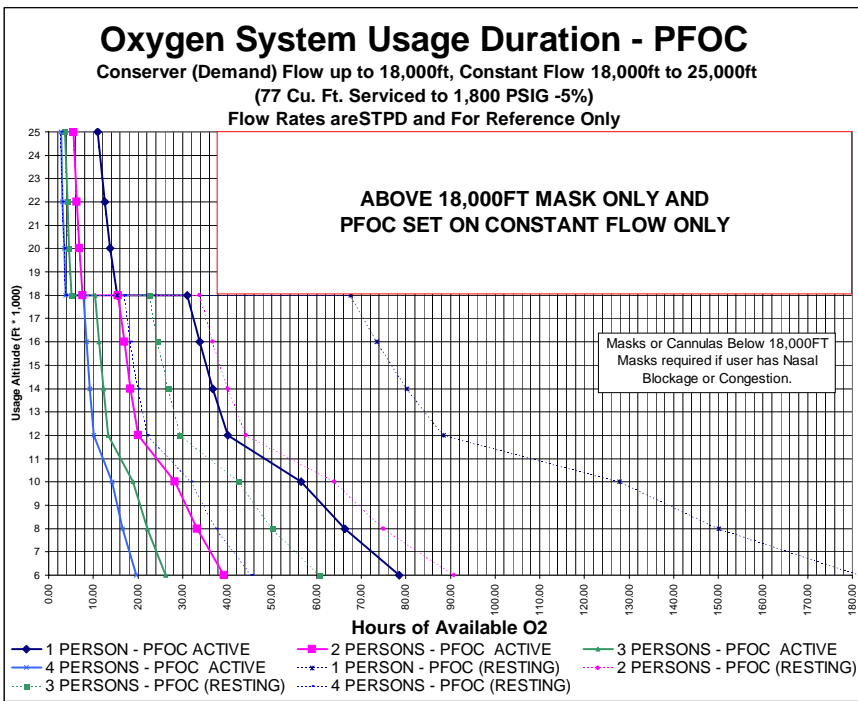


Figure 25 - PreciseFlow Oxygen Conservser

Duration Chart Notes:

- Bottle Capacity has been reduced 5% for safety
- The installation of this equipment does not affect or change the performance characteristics of the airplane, which are detailed in Section 5 of the primary portion of the *Pilot's Operating Handbook*. No change from basic Handbook.

Section 6 – Weight & Balance

If the aircraft is equipped with and the Oxygen System is installed, it is the pilot's responsibility to verify the weight and balance of the aircraft is within limits with the System installed prior to flight.

The weight, arm, and moment for fully charged systems (1800psig) are provided in Table 4. The total weight of oxygen in the system is 6.4lb and the actual weight and moment can be determined by oxygen pressure per Figure 22.

Table 4 - Weight and Balance Information

	Weight - lb	Arm	Moment/1000
Empty	17.4	262.3	4565.7
Full	23.8	265.3	6316.4

Section 7 – System Description

The general operating procedures for use of the Fixed Oxygen System is discussed in the Section 1 - General System Overview of this Supplement.

Section 8 – Handling, Service, & Maintenance

8.1 – Refilling the Oxygen Bottle

1. Aircraft Electrical Power ON. Ensure Oxygen Cockpit Control OFF.
Aircraft Electrical Power OFF.

Locate Refill panel in the aft baggage bulkhead near aircraft center.

Access the filler port and pressure gauge by opening the door cover.

Oxygen regulator and fill port are located in the center of the fuselage towards the aft edge of the opening. Remove Cap.

■ Caution ■

Clean both the oxygen supply line and the filler port to ensure it is clear of oils, dirt, etc., that may create a fire hazard during refilling. Check threads and ensure the filling port fitting threads are not damaged.

2. Connect oxygen cart or oxygen supply line to the AN fitting.
3. Open oxygen supply and slowly, at a rate of 200 psi per minute, fill bottle to 1800 psi maximum.

■ Caution ■

Excessive fill rates create heat build up in the high pressure parts of the System, especially the bottle. Excessive heat build up will result in damage to the bottle, and may lead to fire. Care must be taken during refilling of the Oxygen System.

4. Close oxygen supply.
5. Important: Bleed pressure from supply line.
6. Remove oxygen supply line.
7. Refit cap to fill port.
8. Close door cover.

8.2 – Oxygen Component Cleaning

Periodically clean the oxygen breathing equipment with Purell <http://www.pfizerch.com> or warm water. As you clean the equipment pay close attention to the condition of the lines and silicone moldings to

ensure no tears or kinks have occurred. Carefully restore oxygen components.

8.2.1 – Flowmeter Anti-Static

Periodic anti-static treatment may be required on the flow meter should the ball act 'sticky' or function erratically. This is caused by the handling of the flowmeter and a simple cleaning is required. The use of de-ionized water with a very mild oxygen and breathing safe detergent is needed. Remove the cannula or mask and add a few drops of this solution in the end of the tube and let it reach the tapered tube of the flowmeter. Then run clean oxygen through the flowmeter until dry. The flowmeter is then ready for use

8.3 – Oxygen Bottle Removal

See FAA-Approved Instructions for Continued Airworthiness for the Precise Flight Oxygen System for oxygen bottle removal instructions.

8.4 – Replacement Components

Table 5 – Options/Replacement FAA-Approved Breathing Station Components

PFI P/N	Description
A4 Constant Flowmeter Options	
027N0202-1	A4 Breathing Station Kit with CPC (Oxymizer Cannula and Standard Face Mask)
027N0203-1	A4 Breathing Station Kit with CPC (Oxymizer Cannula and Face Mask with Microphone)
027N0002-1	A4 Assembly with CPC (No Mask or Cannula)
020N0007-1	Standard Cannula
020N0001-1	Oxymizer Cannula
020N0002-1	Standard Facemask
020N0005-1	Facemask with Microphone
A5 Constant Flowmeter Options	
027N0302-1	A5 Breathing Station Kit with CPC (Oxymizer Cannula and Standard Face Mask)
027N0303-1	A5 Breathing Station Kit with CPC (Oxymizer Cannula and Face Mask with Microphone)
027N0003-1	A5 Assembly with CPC (No Mask or Cannula)
020N0007-1	Standard Cannula
020N0001-1	Oxymizer Cannula
020N0002-1	Standard Facemask
020N0005-1	Facemask with Microphone
PreciseFlow® Options	
027N1101-6	PreciseFlow® (PFOC) Breathing Station Kit with Inline Regulator (Dual Lumen Cannula, and Standard PFOC Mask)
027N1102-6	PreciseFlow® (PFOC) Breathing Station Kit with Inline Regulator (Dual Lumen Cannula, and PFOC Mask with Microphone)
027N1002-1	PreciseFlow® (PFOC) with Inline Regulator and CPC (No Mask or Cannula)
020N0050-1	PreciseFlow® (PFOC) Dual Lumen Cannula
020N0060-1	PreciseFlow® (PFOC) Face Mask
020N0070-1	PreciseFlow® (PFOC) Face Mask with Microphone

■ **Note** ■

Constant flow cannulas, and facemasks are NOT compatible with the PreciseFlow® cannulas and facemasks.

This Page Intentionally Left Blank.